

EN

FR

ES

DE

BR

NL

JA


ZH

KO

Multi-Venous IV Training Arm

Male, Female and Pediatric

User Guide

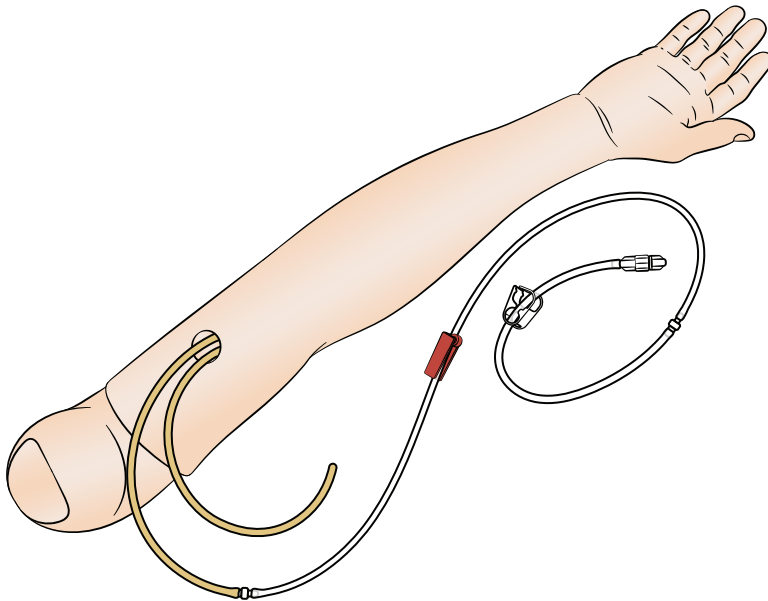

Introduction

EN

The Multi-Venous IV Training Arm is a lifelike arm reproduction with multi-vein system designed for peripheral intravenous therapy. This User Guide covers 3 versions of the Multi-Venous IV Training Arm: Adult Male, Adult Female and Pediatric. Unless otherwise specified, the information in this User Guide applies to all versions.

 Warning

This product contains Natural Rubber Latex which may cause allergic reactions when in contact with humans.

 Caution

Do not use Iodine preparation as this can permanently stain the arm.

 Notes

- Recommended catheter size: 22 gauge or smaller.
- Lubricate with manikin lubricant for easier insertion.
- When excessive leaking occurs, a new skin and multi-vein system should be installed.

FR

The Multi-Venous IV Training Arm is a lifelike arm reproduction with multi-vein system designed for peripheral intravenous therapy. This User Guide covers 3 versions of the Multi-Venous IV Training Arm: Adult Male, Adult Female and Pediatric. Unless otherwise specified, the information in this User Guide applies to all versions.



Warning

This product contains Natural Rubber Latex which may cause allergic reactions when in contact with humans.



Caution

Do not use Iodine preparation as this can permanently stain the arm.



Notes

- Recommended catheter size: 22 gauge or smaller.
- Lubricate with manikin lubricant for easier insertion.
- When excessive leaking occurs, a new skin and multi-vein system should be installed.

ES

The Multi-Venous IV Training Arm is a lifelike arm reproduction with multi-vein system designed for peripheral intravenous therapy. This User Guide covers 3 versions of the Multi-Venous IV Training Arm: Adult Male, Adult Female and Pediatric. Unless otherwise specified, the information in this User Guide applies to all versions.



Warning

This product contains Natural Rubber Latex which may cause allergic reactions when in contact with humans.



Caution

Do not use Iodine preparation as this can permanently stain the arm.



Notes

- Recommended catheter size: 22 gauge or smaller.
- Lubricate with manikin lubricant for easier insertion.
- When excessive leaking occurs, a new skin and multi-vein system should be installed.

DE

The Multi-Venous IV Training Arm is a lifelike arm reproduction with multi-vein system designed for peripheral intravenous therapy. This User Guide covers 3 versions of the Multi-Venous IV Training Arm: Adult Male, Adult Female and Pediatric. Unless otherwise specified, the information in this User Guide applies to all versions.



Warning

This product contains Natural Rubber Latex which may cause allergic reactions when in contact with humans.



Caution

Do not use Iodine preparation as this can permanently stain the arm.

Introduction



Notes

- Recommended catheter size: 22 gauge or smaller.
- Lubricate with manikin lubricant for easier insertion.
- When excessive leaking occurs, a new skin and multi-vein system should be installed.

BR

The Multi-Venous IV Training Arm is a lifelike arm reproduction with multi-vein system designed for peripheral intravenous therapy. This User Guide covers 3 versions of the Multi-Venous IV Training Arm: Adult Male, Adult Female and Pediatric. Unless otherwise specified, the information in this User Guide applies to all versions.



Warning

This product contains Natural Rubber Latex which may cause allergic reactions when in contact with humans.



Caution

Do not use Iodine preparation as this can permanently stain the arm.



Notes

- Recommended catheter size: 22 gauge or smaller.
- Lubricate with manikin lubricant for easier insertion.
- When excessive leaking occurs, a new skin and multi-vein system should be installed.

NL

The Multi-Venous IV Training Arm is a lifelike arm reproduction with multi-vein system designed for peripheral intravenous therapy. This User Guide covers 3 versions of the Multi-Venous IV Training Arm: Adult Male, Adult Female and Pediatric. Unless otherwise specified, the information in this User Guide applies to all versions.



Warning

This product contains Natural Rubber Latex which may cause allergic reactions when in contact with humans.



Caution

Do not use Iodine preparation as this can permanently stain the arm.



Notes

- Recommended catheter size: 22 gauge or smaller.
- Lubricate with manikin lubricant for easier insertion.
- When excessive leaking occurs, a new skin and multi-vein system should be installed.

JA

The Multi-Venous IV Training Arm is a lifelike arm reproduction with multi-vein system designed for peripheral intravenous therapy. This User Guide covers 3 versions of the Multi-Venous IV Training Arm: Adult Male, Adult Female and Pediatric. Unless otherwise specified, the information in this User Guide applies to all versions.



Warning

This product contains Natural Rubber Latex which may cause allergic reactions when in contact with humans.



Caution

Do not use Iodine preparation as this can permanently stain the arm.



Notes

- Recommended catheter size: 22 gauge or smaller.
- Lubricate with manikin lubricant for easier insertion.
- When excessive leaking occurs, a new skin and multi-vein system should be installed.

ZH

The Multi-Venous IV Training Arm is a lifelike arm reproduction with multi-vein system designed for peripheral intravenous therapy. This User Guide covers 3 versions of the Multi-Venous IV Training Arm: Adult Male, Adult Female and Pediatric. Unless otherwise specified, the information in this User Guide applies to all versions.



Warning

This product contains Natural Rubber Latex which may cause allergic reactions when in contact with humans.



Caution

Do not use Iodine preparation as this can permanently stain the arm.



Notes

- Recommended catheter size: 22 gauge or smaller.
- Lubricate with manikin lubricant for easier insertion.
- When excessive leaking occurs, a new skin and multi-vein system should be installed.

KO

The Multi-Venous IV Training Arm is a lifelike arm reproduction with multi-vein system designed for peripheral intravenous therapy. This User Guide covers 3 versions of the Multi-Venous IV Training Arm: Adult Male, Adult Female and Pediatric. Unless otherwise specified, the information in this User Guide applies to all versions.



Warning

This product contains Natural Rubber Latex which may cause allergic reactions when in contact with humans.



Caution

Do not use Iodine preparation as this can permanently stain the arm.




Notes

- Recommended catheter size: 22 gauge or smaller.
- Lubricate with manikin lubricant for easier insertion.
- When excessive leaking occurs, a new skin and multi-vein system should be installed.

Items Included


EN

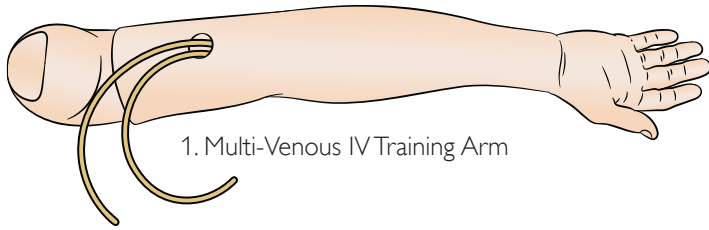


1. Multi-Venous IV Training Arm




2. Replacement Skin



3. Blood Bag



4. Tubing and Clamp




5. Multi-Vein System



6. Manikin
Lubricant




7. Simulated Blood
Concentrate



8. Shoulder Attachment
Hardware



9. Vein Bands (x 4)



10. User Information

FR

1. Multi-Venous IV Training Arm
2. Replacement Skin
3. Blood Bag
4. Tubing and Clamp
5. Multi-Vein System
6. Manikin Lubricant
7. Simulated Blood Concentrate
8. Shoulder Attachment Hardware
9. Vein Bands (x 4)
10. User Information

ES

1. Multi-Venous IV Training Arm
2. Replacement Skin
3. Blood Bag
4. Tubing and Clamp
5. Multi-Vein System
6. Manikin Lubricant
7. Simulated Blood Concentrate
8. Shoulder Attachment Hardware
9. Vein Bands (x 4)
10. User Information

DE

1. Multi-Venous IV Training Arm
2. Replacement Skin
3. Blood Bag
4. Tubing and Clamp
5. Multi-Vein System
6. Manikin Lubricant
7. Simulated Blood Concentrate
8. Shoulder Attachment Hardware
9. Vein Bands (x 4)
10. User Information

BR

1. Multi-Venous IV Training Arm
2. Replacement Skin
3. Blood Bag
4. Tubing and Clamp
5. Multi-Vein System
6. Manikin Lubricant
7. Simulated Blood Concentrate
8. Shoulder Attachment Hardware
9. Vein Bands (x 4)
10. User Information

NL

1. Multi-Venous IV Training Arm
2. Replacement Skin
3. Blood Bag
4. Tubing and Clamp
5. Multi-Vein System
6. Manikin Lubricant
7. Simulated Blood Concentrate
8. Shoulder Attachment Hardware
9. Vein Bands (x 4)
10. User Information

JA

1. Multi-Venous IV Training Arm
2. Replacement Skin
3. Blood Bag
4. Tubing and Clamp
5. Multi-Vein System
6. Manikin Lubricant
7. Simulated Blood Concentrate
8. Shoulder Attachment Hardware
9. Vein Bands (x 4)
10. User Information

ZH

1. Multi-Venous IV Training Arm
2. Replacement Skin
3. Blood Bag
4. Tubing and Clamp
5. Multi-Vein System
6. Manikin Lubricant
7. Simulated Blood Concentrate
8. Shoulder Attachment Hardware
9. Vein Bands (x 4)
10. User Information


KO

1. Multi-Venous IV Training Arm
2. Replacement Skin
3. Blood Bag
4. Tubing and Clamp
5. Multi-Vein System
6. Manikin Lubricant
7. Simulated Blood Concentrate
8. Shoulder Attachment Hardware
9. Vein Bands (x 4)
10. User Information


Overview

EN

Adult Male Multi-Venous IV Arm

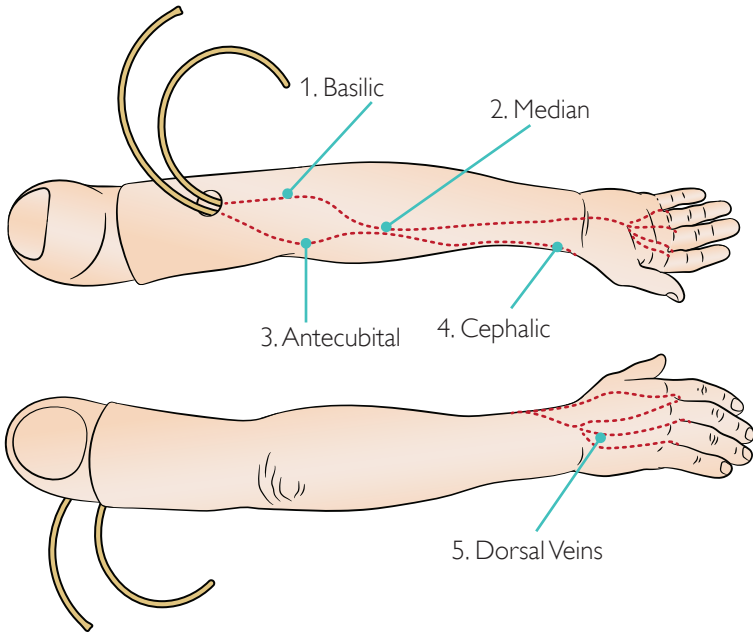

Adult Female / Pediatric Multi-Venous IV Arm

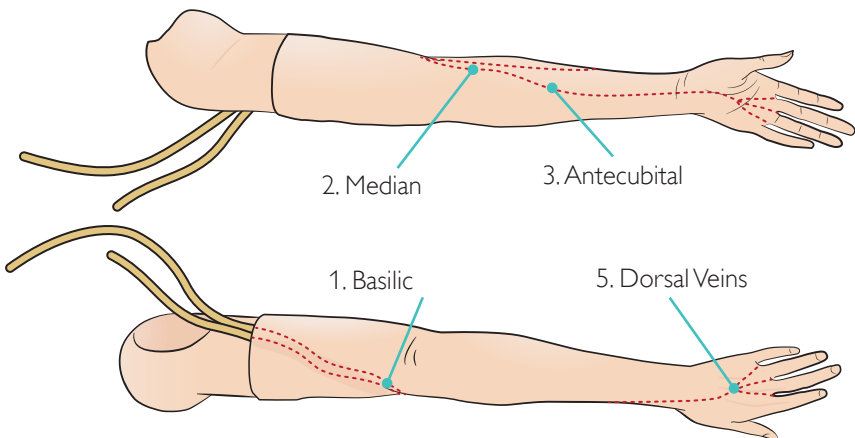

FR

Adult Male Multi-Venous IV Arm
Adult Female / Pediatric Multi-Venous IV Arm

1. Basilic
2. Median
3. Antecubital
4. Cephalic
5. Dorsal Veins

ES

Adult Male Multi-Venous IV Arm
Adult Female / Pediatric Multi-Venous IV Arm

1. Basilic
2. Median
3. Antecubital
4. Cephalic
5. Dorsal Veins

DE

Adult Male Multi-Venous IV Arm
Adult Female / Pediatric Multi-Venous IV Arm

1. Basilic
2. Median
3. Antecubital
4. Cephalic
5. Dorsal Veins

BR

Adult Male Multi-Venous IV Arm
Adult Female / Pediatric Multi-Venous IV Arm

1. Basilic
2. Median
3. Antecubital
4. Cephalic
5. Dorsal Veins

NL

Adult Male Multi-Venous IV Arm
Adult Female / Pediatric Multi-Venous IV Arm

1. Basilic
2. Median
3. Antecubital
4. Cephalic
5. Dorsal Veins

JA

Adult Male Multi-Venous IV Arm
Adult Female / Pediatric Multi-Venous IV Arm

1. Basilic
2. Median
3. Antecubital
4. Cephalic
5. Dorsal Veins

ZH

Adult Male Multi-Venous IV Arm
Adult Female / Pediatric Multi-Venous IV Arm

1. Basilic
2. Median
3. Antecubital
4. Cephalic
5. Dorsal Veins


KO

Adult Male Multi-Venous IV Arm
Adult Female / Pediatric Multi-Venous IV Arm




1. Basilic
2. Median
3. Antecubital
4. Cephalic
5. Dorsal Veins

Setup

1

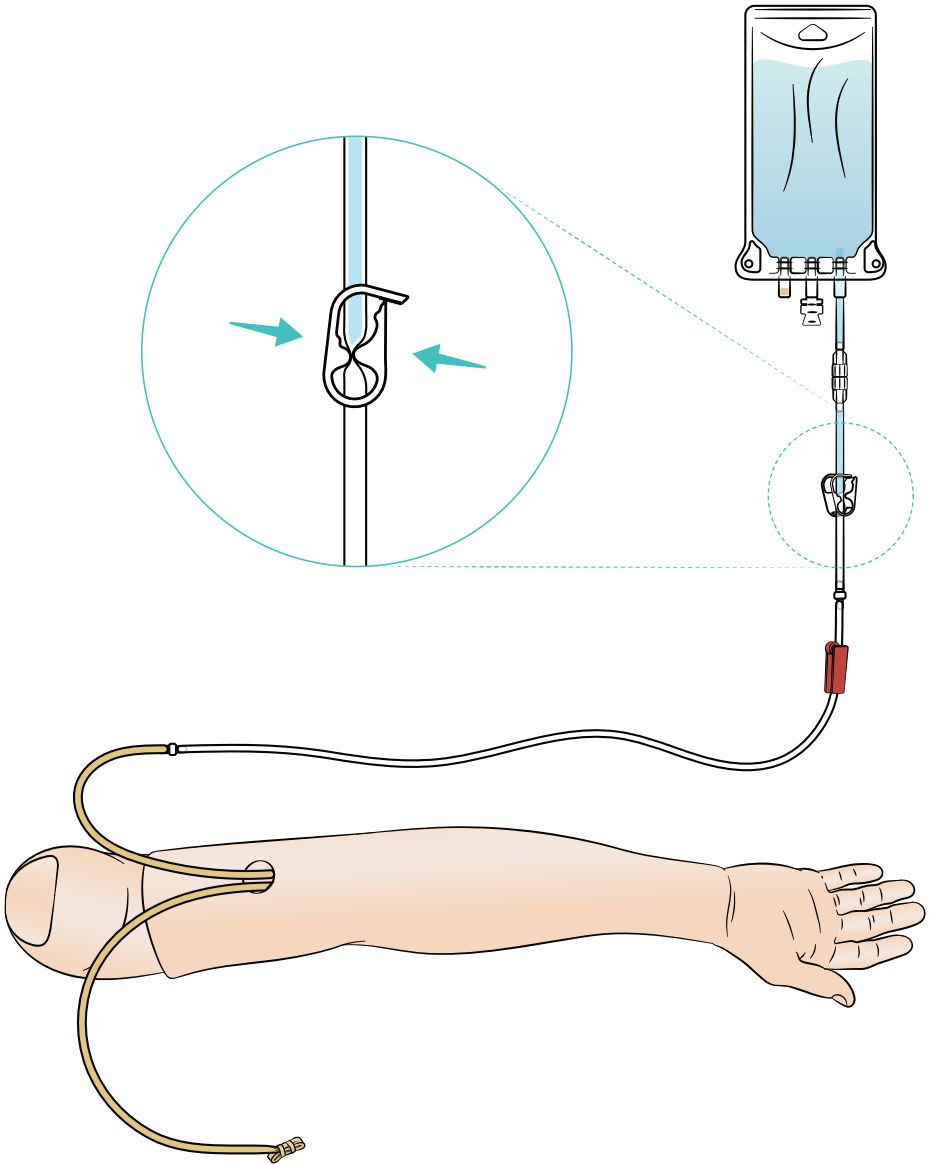


2

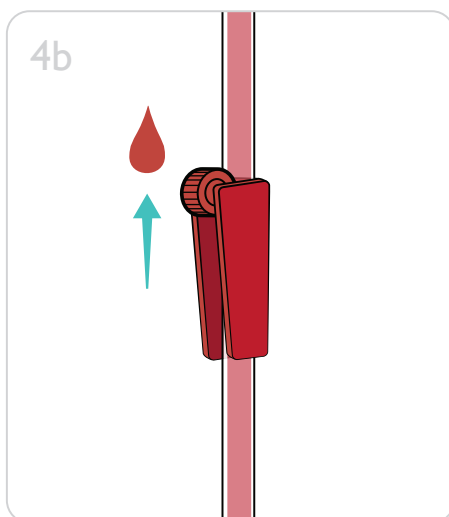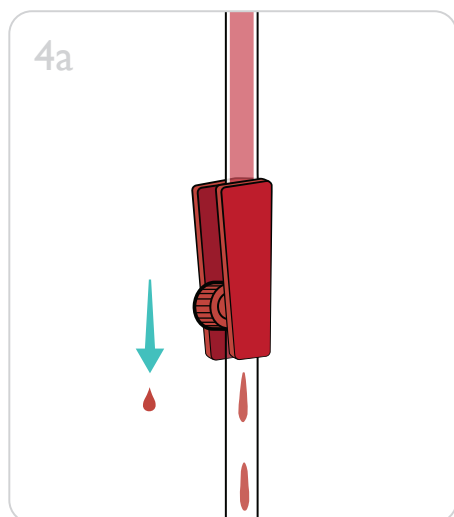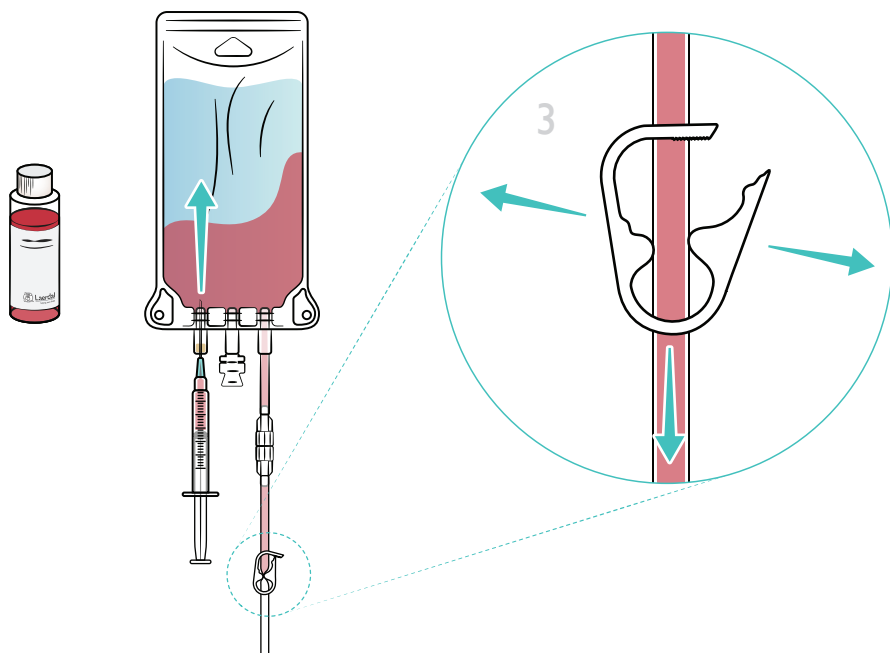


Removing Skin & Vein System


1

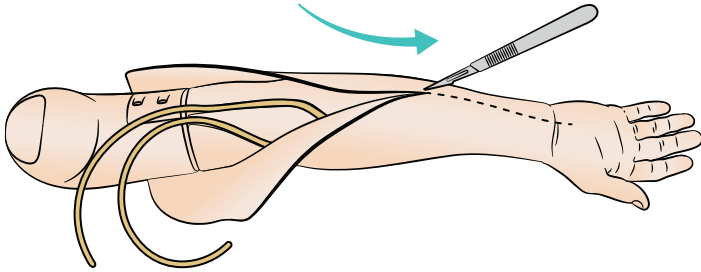


2

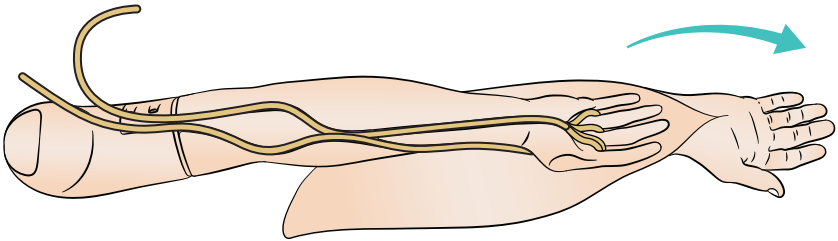



3

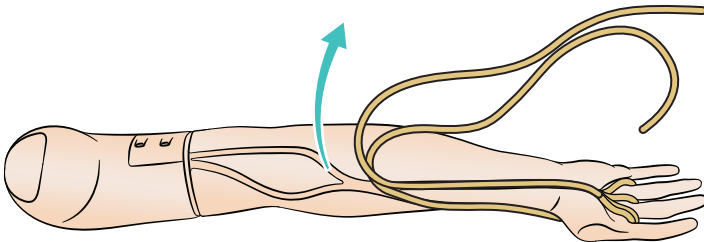

4

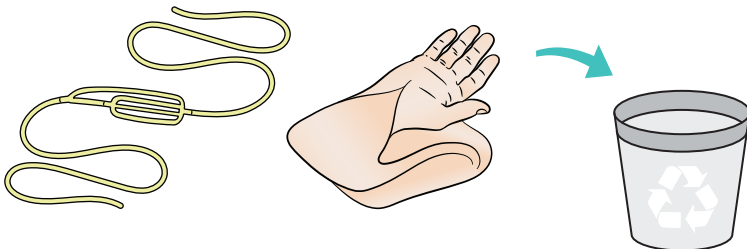

5

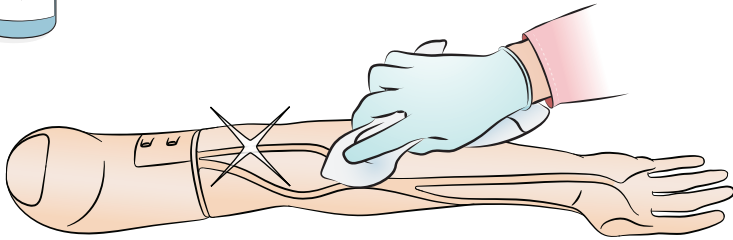

EN



Note

Excess dried glue may need to be scraped away.

FR



Note

Excess dried glue may need to be scraped away.

ES



Note

Excess dried glue may need to be scraped away.

DE



Note

Excess dried glue may need to be scraped away.

BR



Note

Excess dried glue may need to be scraped away.

NL



Note

Excess dried glue may need to be scraped away.

JA



Note

Excess dried glue may need to be scraped away.

ZH



Note

Excess dried glue may need to be scraped away.

KO




Note

Excess dried glue may need to be scraped away.


Replacing Skin & Vein System

6

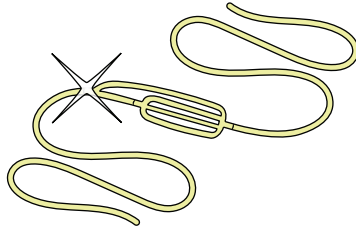


7


2.5 cm / 1 in

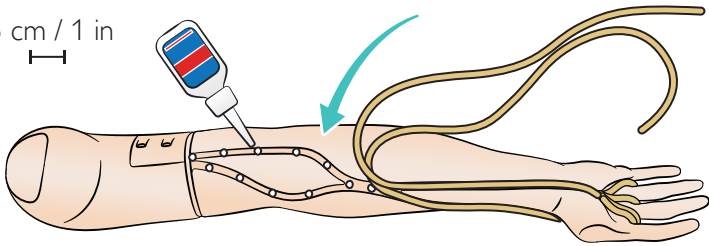

8

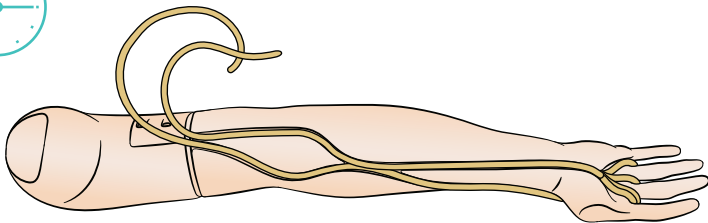

9

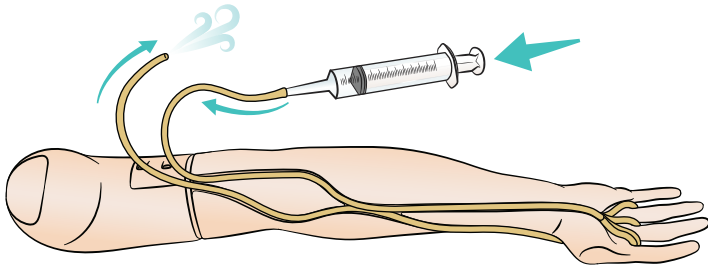

EN

9. Push air through vein with a syringe to check for kinks or blockages.

FR

9. Push air through vein with a syringe to check for kinks or blockages.

NL

9. Push air through vein with a syringe to check for kinks or blockages.

ES

9. Push air through vein with a syringe to check for kinks or blockages.

JA

9. Push air through vein with a syringe to check for kinks or blockages.

DE

9. Push air through vein with a syringe to check for kinks or blockages.

ZH

9. Push air through vein with a syringe to check for kinks or blockages.

BR


9. Push air through vein with a syringe to check for kinks or blockages.

KO

9. Push air through vein with a syringe to check for kinks or blockages.

Replacing Skin & Vein System


10

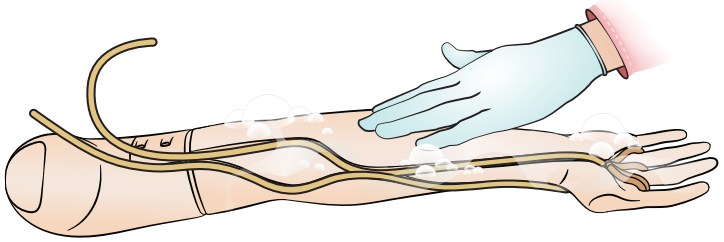


11



12

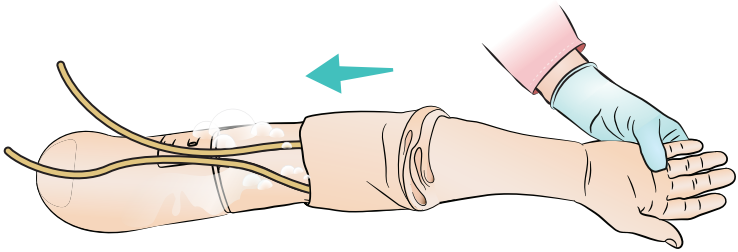

13

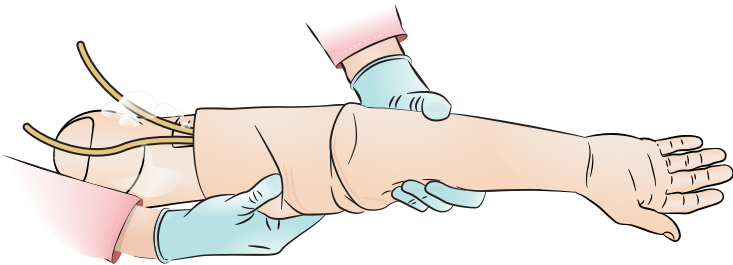

EN

 Notes

- Heat arm skin before replacing on mandrel. This can be done with a hair dryer.
- Male arm skin includes thumb piece.

FR

 Notes

- Heat arm skin before replacing on mandrel. This can be done with a hair dryer.
- Male arm skin includes thumb piece.

JA

 Notes

- Heat arm skin before replacing on mandrel. This can be done with a hair dryer.
- Male arm skin includes thumb piece.

ES

 Notes

- Heat arm skin before replacing on mandrel. This can be done with a hair dryer.
- Male arm skin includes thumb piece.

ZH

 Notes

- Heat arm skin before replacing on mandrel. This can be done with a hair dryer.
- Male arm skin includes thumb piece.

DE

 Notes

- Heat arm skin before replacing on mandrel. This can be done with a hair dryer.
- Male arm skin includes thumb piece.

KO

 Notes

- Heat arm skin before replacing on mandrel. This can be done with a hair dryer.
- Male arm skin includes thumb piece.

BR

 Notes

- Heat arm skin before replacing on mandrel. This can be done with a hair dryer.
- Male arm skin includes thumb piece.

NL

 Notes

- Heat arm skin before replacing on mandrel. This can be done with a hair dryer.
- Male arm skin includes thumb piece.

Care & Maintenance

EN

- Clean arm with mild soap and water after each training session and perform a general inspection regularly.
- Flush veins with water and then air using a slip tip syringe. Disinfect when needed with a mild solution of bleach and water followed by flushing with air.
- If using deltoid injection pad (water only), squeeze water from foam pad after each training session. Allow pad to air dry prior to reinsertion into skin. Dust with talcum powder to aid insertion. Pads may be soaked in a mild solution of bleach and water to prevent mildew or mold. Do not store wet foam pads in the skin.

Cautions

- *Do not submerge arm or other parts in cleaning fluid or water.*
- *Avoid using colored plastic gloves as they may discolor the arm skin. Do not use felt-tipped markers, ink pens, acetone, iodine, or other staining material near the arm. Take care not to place the arm on printed paper, newsprint, or colored paper. Staining may be permanent.*

FR

- Clean arm with mild soap and water after each training session and perform a general inspection regularly.
- Flush veins with water and then air using a slip tip syringe. Disinfect when needed with a mild solution of bleach and water followed by flushing with air.
- If using deltoid injection pad (water only), squeeze water from foam pad after each training session. Allow pad to air dry prior to reinsertion into skin. Dust with talcum powder to aid insertion. Pads may be soaked in a mild solution of bleach and water to prevent mildew or mold. Do not store wet foam pads in the skin.

Cautions

- *Do not submerge arm or other parts in cleaning fluid or water.*
- *Avoid using colored plastic gloves as they may discolor the arm skin. Do not use felt-tipped markers, ink pens, acetone, iodine, or other staining material near the arm. Take care not to place the arm on printed paper, newsprint, or colored paper. Staining may be permanent.*

ES

- Clean arm with mild soap and water after each training session and perform a general inspection regularly.
- Flush veins with water and then air using a slip tip syringe. Disinfect when needed with a mild solution of bleach and water followed by flushing with air.
- If using deltoid injection pad (water only), squeeze water from foam pad after each training session. Allow pad to air dry prior to reinsertion into skin. Dust with talcum powder to aid insertion. Pads may be soaked in a mild solution of bleach and water to prevent mildew or mold. Do not store wet foam pads in the skin.

Cautions

- *Do not submerge arm or other parts in cleaning fluid or water.*
- *Avoid using colored plastic gloves as they may discolor the arm skin. Do not use felt-tipped markers, ink pens, acetone, iodine, or other staining material near the arm. Take care not to place the arm on printed paper, newsprint, or colored paper. Staining may be permanent.*

DE

- Clean arm with mild soap and water after each training session and perform a general inspection regularly.
- Flush veins with water and then air using a slip tip syringe. Disinfect when needed with a mild solution of bleach and water followed by flushing with air.
- If using deltoid injection pad (water only), squeeze water from foam pad after each training session. Allow pad to air dry prior to reinsertion into skin. Dust with talcum powder to aid insertion. Pads may be soaked in a mild solution of bleach and water to prevent mildew or mold. Do not store wet foam pads in the skin.

Cautions

- *Do not submerge arm or other parts in cleaning fluid or water.*
- *Avoid using colored plastic gloves as they may discolor the arm skin. Do not use felt-tipped markers, ink pens, acetone, iodine, or other staining material near the arm. Take care not to place the arm on printed paper, newsprint, or colored paper. Staining may be permanent.*

BR

- Clean arm with mild soap and water after each training session and perform a general inspection regularly.
- Flush veins with water and then air using a slip tip syringe. Disinfect when needed with a mild solution of bleach and water followed by flushing with air.
- If using deltoid injection pad (water only), squeeze water from foam pad after each training session. Allow pad to air dry prior to reinsertion into skin. Dust with talcum powder to aid insertion. Pads may be soaked in a mild solution of bleach and water to prevent mildew or mold. Do not store wet foam pads in the skin.

Cautions

- *Do not submerge arm or other parts in cleaning fluid or water.*
- *Avoid using colored plastic gloves as they may discolor the arm skin. Do not use felt-tipped markers, ink pens, acetone, iodine, or other staining material near the arm. Take care not to place the arm on printed paper, newsprint, or colored paper. Staining may be permanent.*

NL

- Clean arm with mild soap and water after each training session and perform a general inspection regularly.
- Flush veins with water and then air using a slip tip syringe. Disinfect when needed with

Care & Maintenance

a mild solution of bleach and water followed by flushing with air.

- If using deltoid injection pad (water only), squeeze water from foam pad after each training session. Allow pad to air dry prior to reinsertion into skin. Dust with talcum powder to aid insertion. Pads may be soaked in a mild solution of bleach and water to prevent mildew or mold. Do not store wet foam pads in the skin.

Cautions

- *Do not submerge arm or other parts in cleaning fluid or water.*
- *Avoid using colored plastic gloves as they may discolor the arm skin. Do not use felt-tipped markers, ink pens, acetone, iodine, or other staining material near the arm. Take care not to place the arm on printed paper, newsprint, or colored paper. Staining may be permanent.*

JA

- Clean arm with mild soap and water after each training session and perform a general inspection regularly.
- Flush veins with water and then air using a slip tip syringe. Disinfect when needed with a mild solution of bleach and water followed by flushing with air.
- If using deltoid injection pad (water only), squeeze water from foam pad after each training session. Allow pad to air dry prior to reinsertion into skin. Dust with talcum powder to aid insertion. Pads may be soaked in a mild solution of bleach and water to prevent mildew or mold. Do not store wet foam pads in the skin.

Cautions

- *Do not submerge arm or other parts in cleaning fluid or water.*
- *Avoid using colored plastic gloves as they may discolor the arm skin. Do not use felt-tipped markers, ink pens, acetone, iodine, or other staining material near the arm. Take care not to place the arm on printed paper, newsprint, or colored paper. Staining may be permanent.*

ZH

- Clean arm with mild soap and water after each training session and perform a general inspection regularly.
- Flush veins with water and then air using a slip tip syringe. Disinfect when needed with a mild solution of bleach and water followed by flushing with air.
- If using deltoid injection pad (water only), squeeze water from foam pad after each training session. Allow pad to air dry prior to reinsertion into skin. Dust with talcum powder to aid insertion. Pads may be soaked in a mild solution of bleach and water to prevent mildew or mold. Do not store wet foam pads in the skin.

Cautions

- *Do not submerge arm or other parts in cleaning fluid or water.*
- *Avoid using colored plastic gloves as they may discolor the arm skin. Do not use felt-tipped markers, ink pens, acetone, iodine, or other staining material near the arm. Take care not to place the arm on printed paper, newsprint, or colored paper. Staining may be permanent.*

KO

- Clean arm with mild soap and water after each training session and perform a general inspection regularly.
- Flush veins with water and then air using a slip tip syringe. Disinfect when needed with a mild solution of bleach and water followed by flushing with air.
- If using deltoid injection pad (water only), squeeze water from foam pad after each training session. Allow pad to air dry prior to reinsertion into skin. Dust with talcum powder to aid insertion. Pads may be soaked in a mild solution of bleach and water to prevent mildew or mold. Do not store wet foam pads in the skin.

Cautions

- *Do not submerge arm or other parts in cleaning fluid or water.*
- *Avoid using colored plastic gloves as they may discolor the arm skin. Do not use felt-tipped markers, ink pens, acetone, iodine, or other staining material near the arm. Take care not to place the arm on printed paper, newsprint, or colored paper. Staining may be permanent.*

Important Information

EN

Specifications			
Storage temperature	4 °C to 40 °C (39 °F to 104 °F)		
Operating temperature	-15 °C to 50 °C (5 °F to 122 °F)		
Humidity	20% - 90% (non-condensing)		
	Male Arm	Female Arm	Pediatric Arm
Weight	1.7 kg (3.7 lbs)	1.79 kg (3.95 lbs)	0.91 kg (2 lbs)
Dimension	72.4 cm (28.5 inches)	73.7 cm (29 inches)	51.44 cm (20.25 inches)
Store indoors and not in direct sunlight			

Replacement Parts

For latest replacement parts and accessories, please see www.laerdal.com



Warnings and Cautions

A Warning states a condition, hazard, or unsafe practice that can result in serious personal injury or death.

A Caution states a condition, hazard, or unsafe practice that can result in minor personal injury or damage to the product.



Notes

A note states important information about the product or its operations.

FR

Specifications			
Storage temperature	4 °C to 40 °C (39 °F to 104 °F)		
Operating temperature	-15 °C to 50 °C (5 °F to 122 °F)		
Humidity	20% - 90% (non-condensing)		
	Male Arm	Female Arm	Pediatric Arm
Weight	1.7 kg (3.7 lbs)	1.79 kg (3.95 lbs)	0.91 kg (2 lbs)
Dimension	72.4 cm (28.5 inches)	73.7 cm (29 inches)	51.44 cm (20.25 inches)
Store indoors and not in direct sunlight			

Replacement Parts

For latest replacement parts and accessories, please see www.laerdal.com



Warnings and Cautions

A Warning states a condition, hazard, or unsafe practice that can result in serious personal injury or death.

A Caution states a condition, hazard, or unsafe practice that can result in minor personal injury or damage to the product.



Notes

A note states important information about the product or its operations.

ES

Specifications			
Storage temperature	4 °C to 40 °C (39 °F to 104 °F)		
Operating temperature	-15 °C to 50 °C (5 °F to 122 °F)		
Humidity	20% - 90% (non-condensing)		
	Male Arm	Female Arm	Pediatric Arm
Weight	1.7 kg (3.7 lbs)	1.79 kg (3.95 lbs)	0.91 kg (2 lbs)
Dimension	72.4 cm (28.5 inches)	73.7 cm (29 inches)	51.44 cm (20.25 inches)
Store indoors and not in direct sunlight			

Replacement Parts

For latest replacement parts and accessories, please see www.laerdal.com



Warnings and Cautions

A Warning states a condition, hazard, or unsafe practice that can result in serious personal injury or death.

A Caution states a condition, hazard, or unsafe practice that can result in minor personal injury or damage to the product.



Notes

A note states important information about the product or its operations.

DE

Specifications			
Storage temperature	4 °C to 40 °C (39 °F to 104 °F)		
Operating temperature	-15 °C to 50 °C (5 °F to 122 °F)		
Humidity	20% - 90% (non-condensing)		
	Male Arm	Female Arm	Pediatric Arm
Weight	1.7 kg (3.7 lbs)	1.79 kg (3.95 lbs)	0.91 kg (2 lbs)
Dimension	72.4 cm (28.5 inches)	73.7 cm (29 inches)	51.44 cm (20.25 inches)
Store indoors and not in direct sunlight			

Replacement Parts

For latest replacement parts and accessories, please see www.laerdal.com



Warnings and Cautions

A Warning states a condition, hazard, or unsafe practice that can result in serious personal injury or death.

A Caution states a condition, hazard, or unsafe practice that can result in minor personal injury or damage to the product.



Notes

A note states important information about the product or its operations.

Important Information

BR

Specifications			
Storage temperature	4 °C to 40 °C (39 °F to 104 °F)		
Operating temperature	-15 °C to 50 °C (5 °F to 122 °F)		
Humidity	20% - 90% (non-condensing)		
	Male Arm	Female Arm	Pediatric Arm
Weight	1.7 kg (3.7 lbs)	1.79 kg (3.95 lbs)	0.91 kg (2 lbs)
Dimension	72.4 cm (28.5 inches)	73.7 cm (29 inches)	51.44 cm (20.25 inches)
Store indoors and not in direct sunlight			

Replacement Parts

For latest replacement parts and accessories, please see www.laerdal.com



Warnings and Cautions

A Warning states a condition, hazard, or unsafe practice that can result in serious personal injury or death.

A Caution states a condition, hazard, or unsafe practice that can result in minor personal injury or damage to the product.



Notes

A note states important information about the product or its operations.

NL

Specifications			
Storage temperature	4 °C to 40 °C (39 °F to 104 °F)		
Operating temperature	-15 °C to 50 °C (5 °F to 122 °F)		
Humidity	20% - 90% (non-condensing)		
	Male Arm	Female Arm	Pediatric Arm
Weight	1.7 kg (3.7 lbs)	1.79 kg (3.95 lbs)	0.91 kg (2 lbs)
Dimension	72.4 cm (28.5 inches)	73.7 cm (29 inches)	51.44 cm (20.25 inches)
Store indoors and not in direct sunlight			

Replacement Parts

For latest replacement parts and accessories, please see www.laerdal.com



Warnings and Cautions

A Warning states a condition, hazard, or unsafe practice that can result in serious personal injury or death.

A Caution states a condition, hazard, or unsafe practice that can result in minor personal injury or damage to the product.



Notes

A note states important information about the product or its operations.

JA

Specifications			
Storage temperature	4 °C to 40 °C (39 °F to 104 °F)		
Operating temperature	-15 °C to 50 °C (5 °F to 122 °F)		
Humidity	20% - 90% (non-condensing)		
	Male Arm	Female Arm	Pediatric Arm
Weight	1.7 kg (3.7 lbs)	1.79 kg (3.95 lbs)	0.91 kg (2 lbs)
Dimension	72.4 cm (28.5 inches)	73.7 cm (29 inches)	51.44 cm (20.25 inches)
Store indoors and not in direct sunlight			

Replacement Parts

For latest replacement parts and accessories, please see www.laerdal.com



Warnings and Cautions

A Warning states a condition, hazard, or unsafe practice that can result in serious personal injury or death.

A Caution states a condition, hazard, or unsafe practice that can result in minor personal injury or damage to the product.



Notes

A note states important information about the product or its operations.

ZH

Specifications			
Storage temperature	4 °C to 40 °C (39 °F to 104 °F)		
Operating temperature	-15 °C to 50 °C (5 °F to 122 °F)		
Humidity	20% - 90% (non-condensing)		
	Male Arm	Female Arm	Pediatric Arm
Weight	1.7 kg (3.7 lbs)	1.79 kg (3.95 lbs)	0.91 kg (2 lbs)
Dimension	72.4 cm (28.5 inches)	73.7 cm (29 inches)	51.44 cm (20.25 inches)
Store indoors and not in direct sunlight			

Replacement Parts

For latest replacement parts and accessories, please see www.laerdal.com



Warnings and Cautions

A Warning states a condition, hazard, or unsafe practice that can result in serious personal injury or death.

A Caution states a condition, hazard, or unsafe practice that can result in minor personal injury or damage to the product.



Notes

A note states important information about the product or its operations.

Important Information

KO

Specifications			
Storage temperature	4 °C to 40 °C (39 °F to 104 °F)		
Operating temperature	-15 °C to 50 °C (5 °F to 122 °F)		
Humidity	20% - 90% (non-condensing)		
	Male Arm	Female Arm	Pediatric Arm
Weight	1.7 kg (3.7 lbs)	1.79 kg (3.95 lbs)	0.91 kg (2 lbs)
Dimension	72.4 cm (28.5 inches)	73.7 cm (29 inches)	51.44 cm (20.25 inches)
Store indoors and not in direct sunlight			

Replacement Parts

For latest replacement parts and accessories, please see www.laerdal.com

Warnings and Cautions

A Warning states a condition, hazard, or unsafe practice that can result in serious personal injury or death.

A Caution states a condition, hazard, or unsafe practice that can result in minor personal injury or damage to the product.

Notes

A note states important information about the product or its operations.

EN

Global Warranty

Refer to the Laerdal Global Warranty for terms and conditions. For more information visit www.laerdal.com

FR

Global Warranty

Refer to the Laerdal Global Warranty for terms and conditions. For more information visit www.laerdal.com

ES

Global Warranty

Refer to the Laerdal Global Warranty for terms and conditions. For more information visit www.laerdal.com

DE

Global Warranty

Refer to the Laerdal Global Warranty for terms and conditions. For more information visit www.laerdal.com

BR

Global Warranty

Refer to the Laerdal Global Warranty for terms and conditions. For more information visit www.laerdal.com

NL

Global Warranty

Refer to the Laerdal Global Warranty for terms and conditions. For more information visit www.laerdal.com

JA

Global Warranty

Refer to the Laerdal Global Warranty for terms and conditions. For more information visit www.laerdal.com

ZH

Global Warranty

Refer to the Laerdal Global Warranty for terms and conditions. For more information visit www.laerdal.com

KO

Global Warranty

Refer to the Laerdal Global Warranty for terms and conditions. For more information visit www.laerdal.com

© 2019 Laerdal Medical AS. All rights reserved.

Manufactured in USA for:
Laerdal Medical AS
P.O. Box 377, Tanke Svilandsgate 30, 4002 Stavanger, Norway
T: (+47) 51 51 17 00

Printed in USA

20-16104 Rev A

www.laerdal.com



Laerdal
helping save lives